





# Quick Start Guide


1

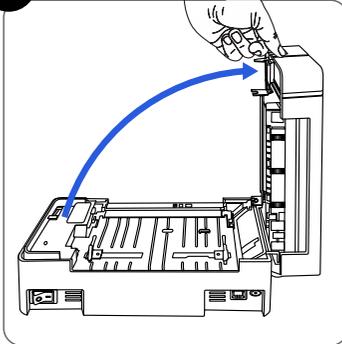


2

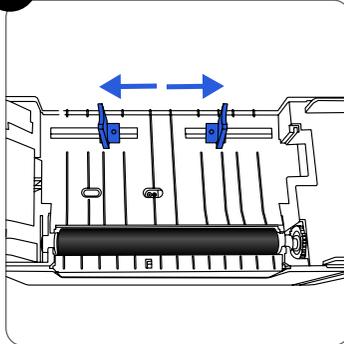


3

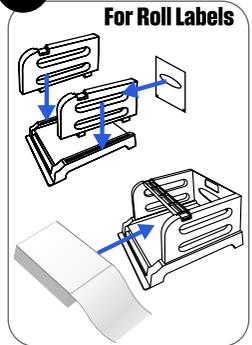


4

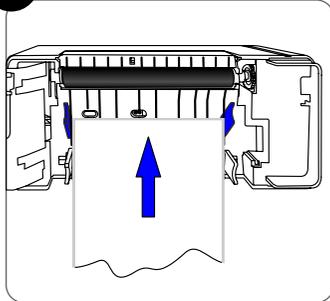


5

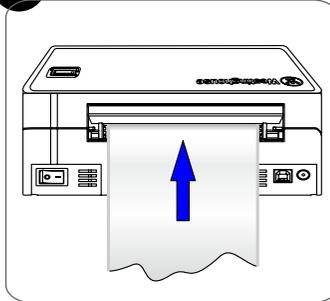


6

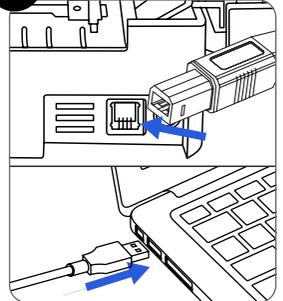

7

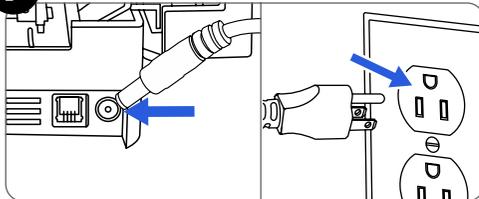

8



9




Please read manual carefully, if you are having set-up issues please contact us:

(877) 474-4900  
support@tps.westinghouse.com



# Operation and Calibration of Labels

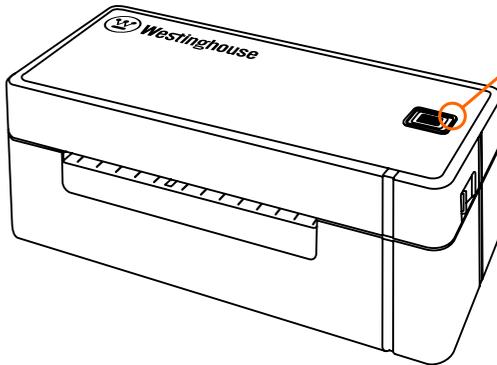

## Feed Button



### Solid Red

which is cover open / out of paper / or printhead over heating






### Solid Green

which is ready to print. Press to feed label.

## How to manually recalibrate the printer:

Before turning the printer on, make sure the labels are loaded properly. Turn the printer on, then press and hold the top feed button until you hear the first beep and release. The printer will automatically begin calibrating. Once calibration is complete, the top indicator light will turn solid green, and the label will stop at the front edge of the printer, indicating it is ready to print.

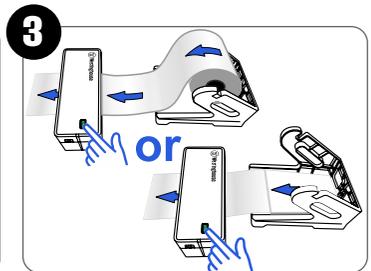

Please read manual carefully, if you are having set-up issues please contact us:

**(877) 474-4900**  
[support@tps.westinghouse.com](mailto:support@tps.westinghouse.com)